

# Electronic Instructions for Use

eIFU

Trauma and  
Extremities

Instructions for use of T&E products  
are available on the **Stryker eIFU website**

**stryker**



**www.ifu.stryker.com**

**stryker**

**About Stryker**

Sehr geehrte Kunden,

Willkommen auf der Website für elektronische Gebrauchsanweisungen (eIFU) von Stryker. Von dieser Seite können Sie anhand der folgenden Schritte unsere elektronische Übersetzung von Stryker-Produktgebrauchsanweisungen herunterladen.

Sie geben die die Produktreferenznummer (REF) die EAN-GTIN oder den KeyCode ein und klicken Sie auf "SEARCH", um die gewünschte Gebrauchsanweisung zu finden. Wenn Sie sich zu einer Information ausgliedern dieser Suchergebnisse.

**Direkter Download** **Erweiterte Suche**

Geben Sie die Produktreferenznummer (REF) die EAN-GTIN (Barcode) oder den KeyCode ein und drücken Sie „SEARCH“

SEARCH Q

REF: 9910515  
REF: 9910515  
(01)12345678912345 (17)21  
GTIN: 12345678912345

Keycode: 123456

Keycode: 123456

Die Übersetzung beim Download der Gebrauchsanweisung zu erhalten, kontaktieren Sie inf@stryker.com

**stryker**

**Instrument** **EN**

**INSTRUCTIONS FOR USE**

L22010584 Rev. AA, 06-2016

Manufacturer:  
Stryker Trauma GmbH  
Professors-Kirchhof-Str. 1-5  
24122 Sankt-Katharinen, Germany  
Phone: +49 (0) 4348 / 702 0  
Fax: +49 (0) 4348 / 702 172

Contact Us: 01-814-18 Rev 2  
Copyright © 2016 Stryker

CE 0123



Environmental aspect – less paper, possible smaller packaging sizes.



Easier version control – latest version always available



Single repository for the whole Stryker T&E portfolio.

Additional labeling available:

- ✓ eGlossary (symbol description)
- ✓ Operative Technique (surgery steps)
- ✓ The Instructions for Cleaning, Sterilization, Inspection and Maintenance
- ✓ Assembly/Disassembly instructions.

# How to know if an IFU is available electronically

Look for the **eIFU indicator** on the product label:



[www.ifu.stryker.com](http://www.ifu.stryker.com)

REF ZZZZZZZZZZ LOT Z999999 **stryker**



(01)000000000000(10)Z999999

VariAx® 2 Compression Systemerweiterung auf 50 ste Ø4.3mm x 262mm,AO 5.0mm Locking Set

**Dorsal DR Plate, narrow, left, long**

Plaque RD dorsale, étroite, gche, longue  
Dorsale DR-Platte, schmal, links, lang  
Placca DR dorsale, stretta, SX, lunga  
Placa DR dorsal, estr., izquierda, larga  
Placa dorsal RD, estreita, esq., longa  
Dorsale DR-plaat, smal, links, lang  
Dorsal DR-platta, smal, vänster, lang  
Dorsal DR-plade, smal, venstre, lang

Dorsal DR-plate, smal, venstre, lang  
Dors. DR-levy, kap, vas, pitkä  
Grzb.płytką dyst.prom.,wąska,lewa,długa  
Ραχιαία πλάκα DR, στενή, αριστ., μακριά  
背側椎骨远端接骨板, 窄型, 左, 长  
등쪽 DR 플레이트, 내로우, 좌, 장형  
Dorsal DR Plak, dar, sol, uzun



2017-12-05  
Humanitarian Use Device

Made in xxxxx  
Material1\_012345678901234

 [www.ifu.stryker.com](http://www.ifu.stryker.com)

QTY 10  
U\_V06130\_07.lab



CE 0123


Stryker GmbH  
Bohnackerweg 1  
2545 Selzach, Switzerland  
U.S. Pat. No: [www.stryker.com/patents](http://www.stryker.com/patents)

Additional information are on the product packaging

stryker

On a Supplemental label

On the inner pages of a peel off label

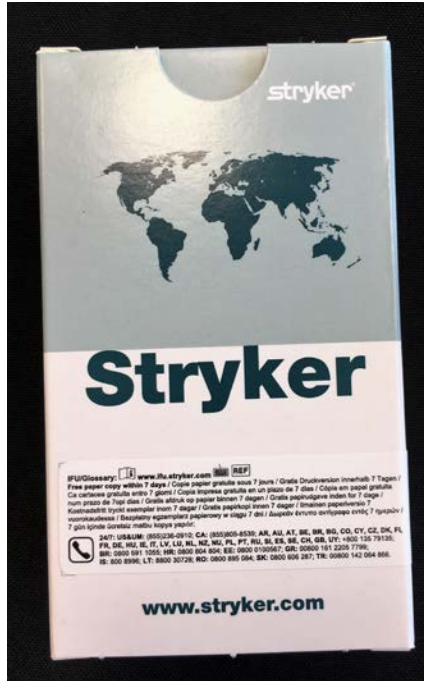

OR





- **Hardware requirements**


- Availability of a Computer/Tablet/Smartphone
- Internet connection

- **Software requirements**


- A web browser (MS Internet Explorer, Mozilla Firefox, Google Chrome).
- A PDF viewer to display and open downloaded eIFUs. A free version of the Adobe PDF viewer can be downloaded here: <https://www.adobe.com/>.

# How to find an eIFU for a product: direct search 1/2

1. Go to [www.ifu.stryker.com](http://www.ifu.stryker.com)

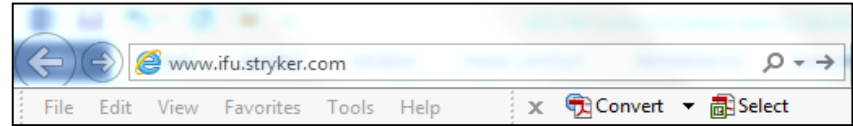


2. On the home page of the Stryker eIFU website, select your preferred language (if not done automatically by the browser)



3. Enter the article number (REF), or the GTIN number (the digits below the barcode, between the two numbers in brackets) on the search field of the Direct download tab



4. Click on the search button to show the results

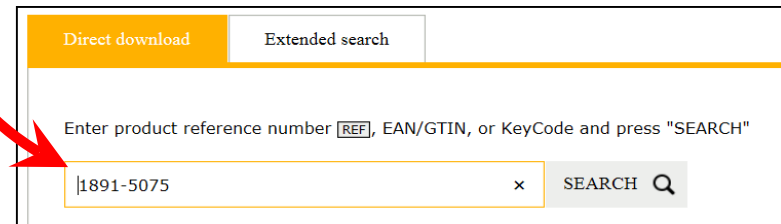

# How to find an eIFU for a product: direct search 2/2

4. Click on the document and language of your choice

Direct download | Extended search

### Locking Screw, Partially Threaded

GTIN : 07613153179009  
REF : 1891-5075

L22000007 Non-Active Implant		L22000007
Current version: AA		2016/01/01
Dansk / DA - Danish	<b>Deutsch / DE - German</b>	English / EN - English
Español / ES - Spanish	Français / FR - French	Italiano / IT - Italian
Nederlands / NL - Dutch	Norsk / NO - Norwegian	Polski / PL - Polish
Português / PT - Portuguese	Suomeksi / FI - Finnish	Svenska / SV - Swedish
Türkçe / TR - Turkish	Ελληνικά / EL - Greek	

5. Enter the security code shown in the picture at the top of the page
6. Click on “download PDF”
7. Accept the pop-up message to confirm version control

The pdf file opens in your computer or digital device

stryker

### Locking Screw, Partially Threaded - 07613153179009

GTIN : 07613153179009 IFU : L22000007 Non-Active Implant - L22000007  
REF : 1891-5075 i : AA

822085

Geben Sie den Code ein PDF herunterladen (268 Kb)

### Confirm version




If saving this Instructions for Use please confirm you have the most up to date version prior to use.

Acknowledge and download



# How to find an eIFU for a product: extended search 1/2

1. In the search field of the Extended search tab, enter any key word describing the product you are searching for, and select a Division
2. Click on the search button to show the results.
3. On the result page, click on the desired item, and you are redirected to the dedicated product page listing all the associated labeling documents

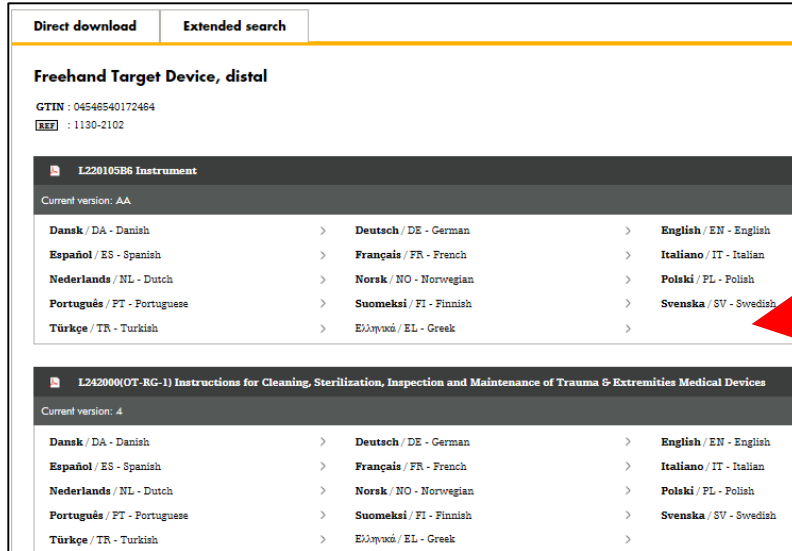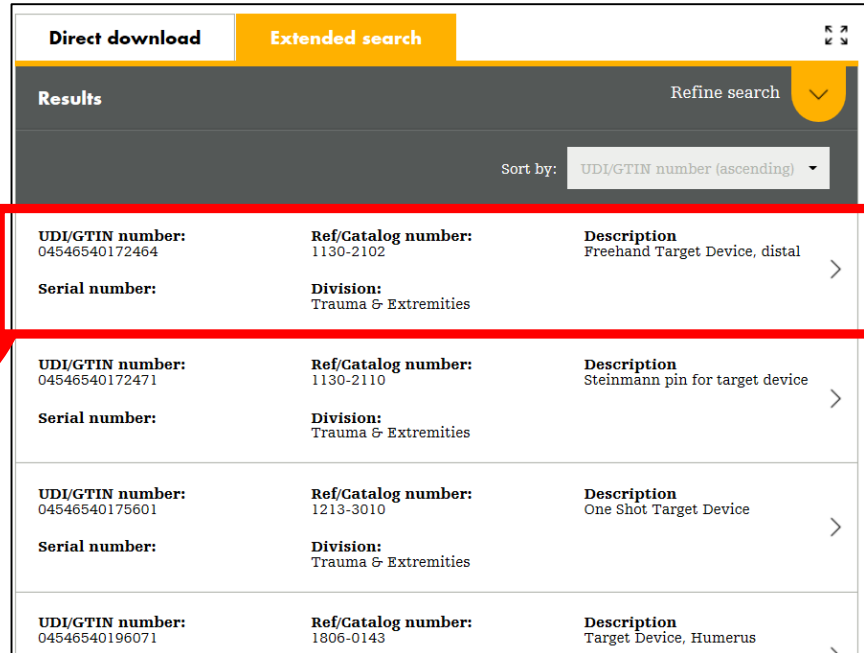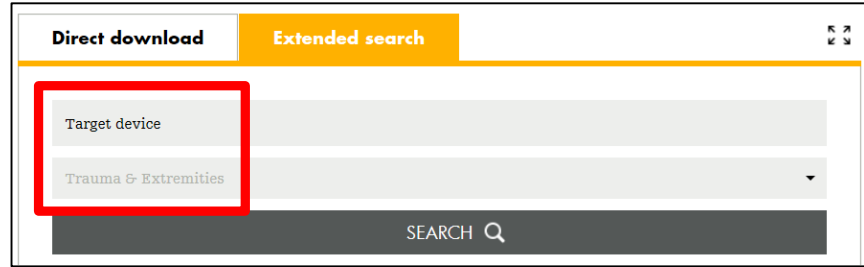

# How to find an eIFU for a product: **extended search** 2/2

5. Click on the document and language of your choice.
6. Enter the security code shown in the picture at the top of the page
7. Click on “download PDF”
8. Accept the pop-up message to confirm version control

The document opens on your computer or digital device.

Direct download | Extended search

---

**Freehand Target Device, distal**

GTIN : 04546540172464  
REF : 1130-2102

**L220105B6 Instrument**

Current version: AA

Dansk / DA - Danish	>	Deutsch / DE - German	>	<b>English / EN - English</b>
Español / ES - Spanish	>	Français / FR - French	>	Italiano / IT - Italian
Nederlands / NL - Dutch	>	Norsk / NO - Norwegian	>	Polski / PL - Polish
Português / PT - Portuguese	>	Suomeksi / FI - Finnish	>	Svenska / SV - Swedish
Türkçe / TR - Turkish	>	Ελληνικά / EL - Greek	>	

**L242000(OT-RG-1) Instructions for Cleaning, Sterilization, Inspection and Maintenance of Trauma & Extremities Medical Devices**

stryker

Instrument EN

INSTRUCTIONS FOR USE

L220105B6 Rev. AA, 06/2016

Manufactured by  
stryker Trauma System  
Parsippany, NJ, USA

© 2016 Stryker Corporation  
All rights reserved.

CE 0123

**Freehand Target Device, distal - 04546540172464**

GTIN : 04546540172464 IFU : L220105B6 Instrument - L220105B6  
REF : 1130-2102 : AA

please enter the code Download PDF (571 Kb)

Note: PDF files require Adobe Acrobat which can be downloaded from the Adobe website. Click [here](#) to download

**Confirm version**

If saving this Instructions for Use please confirm you have the most up to date version prior to use.

Acknowledge and download

Deutsch / DE - German	>	English / EN - English
Français / FR - French	>	Italiano / IT - Italian
Norsk / NO - Norwegian	>	Polski / PL - Polish
Suomeksi / FI - Finnish	>	Svenska / SV - Swedish
Ελληνικά / EL - Greek	>	



AR AU AT BE  
BR BG CO CY  
CZ DK FI FR  
DE HU IE IT  
LV LU NL NZ  
NU PL PT RU  
SI ES SE CH  
GB UY  
+800 135 79135

<b>US UM</b>	(855)236-0910
<b>CA</b>	(855)805-8539
<b>BR</b>	0800 591 1055
<b>HR</b>	0800 804 804
<b>EE</b>	0800 0100567
<b>GR</b>	00800 161 2205 7799
<b>IS</b>	800 8996
<b>LT</b>	8800 30728
<b>RO</b>	0800 895 084
<b>SK</b>	0800 606 287
<b>TR</b>	00800 142 064 866
<b>SG</b>	800 101 3366
<b>VN</b>	122 80297

## To order a free paper copy, you need a telephone:

1. Consult the eIFU information on the product package.
2. Locate the call center phone number of your geographical area (indicated by the two digits country codes).  
The call center is available 24 hours a day, 7 days a week.
  1. Call the number and follow the operator instructions.
  2. Provide the address where you would like to receive the paper copy of your eIFU.

The paper copy of the eIFU will be delivered at the indicated address without any additional cost, and within 7 days.

## 1. How do I enter the article number (REF)?

As it is shown on the label, including any special characters (dash, slash, period, etc.), for example:

181755

1891-5075

1847-0003S

99-0028/11F

WA/B-NL

500.220

## 2. Why there are no results shown?

Not all Stryker T&E products have an IFU. If there is no IFU associated with a certain product, the following message is displayed: “document not found”

## 3. Who do I contact if I need assistance for the download?

Please contact [info@e-labeling.eu](mailto:info@e-labeling.eu), or your sales representative

## 4. When is the call center available to order a free paper copy of the eIFU?

24 hours a day, 7 days a week