


ReUnion[®] S

Shoulder System

Tray layout card



Tray layout sheet – ReUnion S Shoulder System

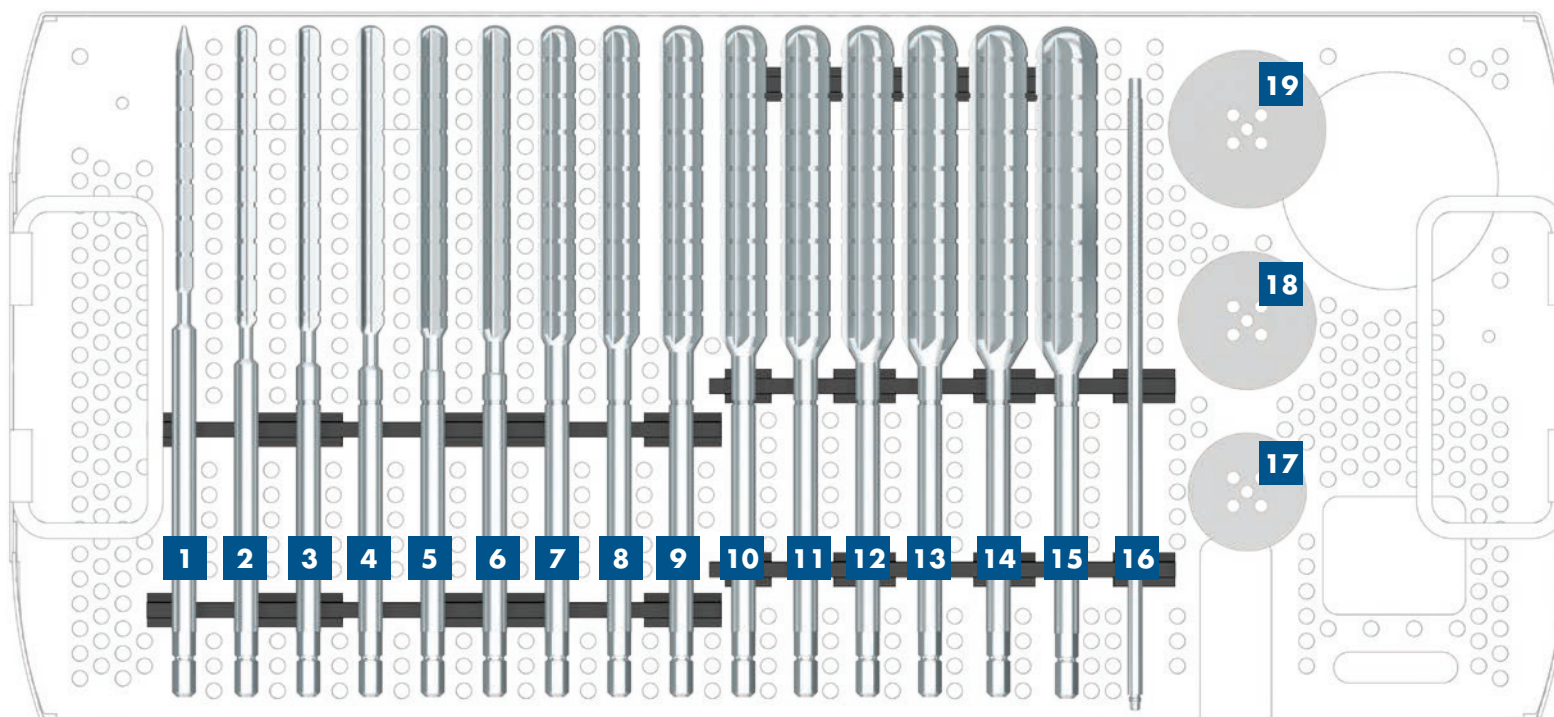


Ref #	Description	Size	Qty.
1 5901-4001	ReUnion S Starter awl	6mm	1
2 5901-4007	ReUnion S Humeral reamer	7mm	1
3 5901-4008	ReUnion S Humeral reamer	8mm	1
4 5901-4009	ReUnion S Humeral reamer	9mm	1
5 5901-4010	ReUnion S Humeral reamer	10mm	1
6 5901-4011	ReUnion S Humeral reamer	11mm	1
7 5901-4012	ReUnion S Humeral reamer	12mm	1
8 5901-4013	ReUnion S Humeral reamer	13mm	1
9 5901-4014	ReUnion S Humeral reamer	14mm	1
10 5901-4015	ReUnion S Humeral reamer	15mm	1

Ref #	Description	Size	Qty.
11 5901-4016	ReUnion S Humeral reamer	16mm	1
12 5901-4017	ReUnion S Humeral reamer	17mm	1
13 5901-4018	ReUnion S Humeral reamer	18mm	1
14 5901-4019	ReUnion S Humeral reamer	19mm	1
15 5901-4020	ReUnion S Humeral reamer	20mm	1
16 5901-1103	Version rod		1
17 5901-4002	Humeral protector plate	Small	1
18 5901-4003	Humeral protector plate	Medium	1
19 5901-4004	Humeral protector plate	Large	1
5901-1224	ReUnion S Shoulder Insert		1



Tray layout sheet – ReUnion S Shoulder System

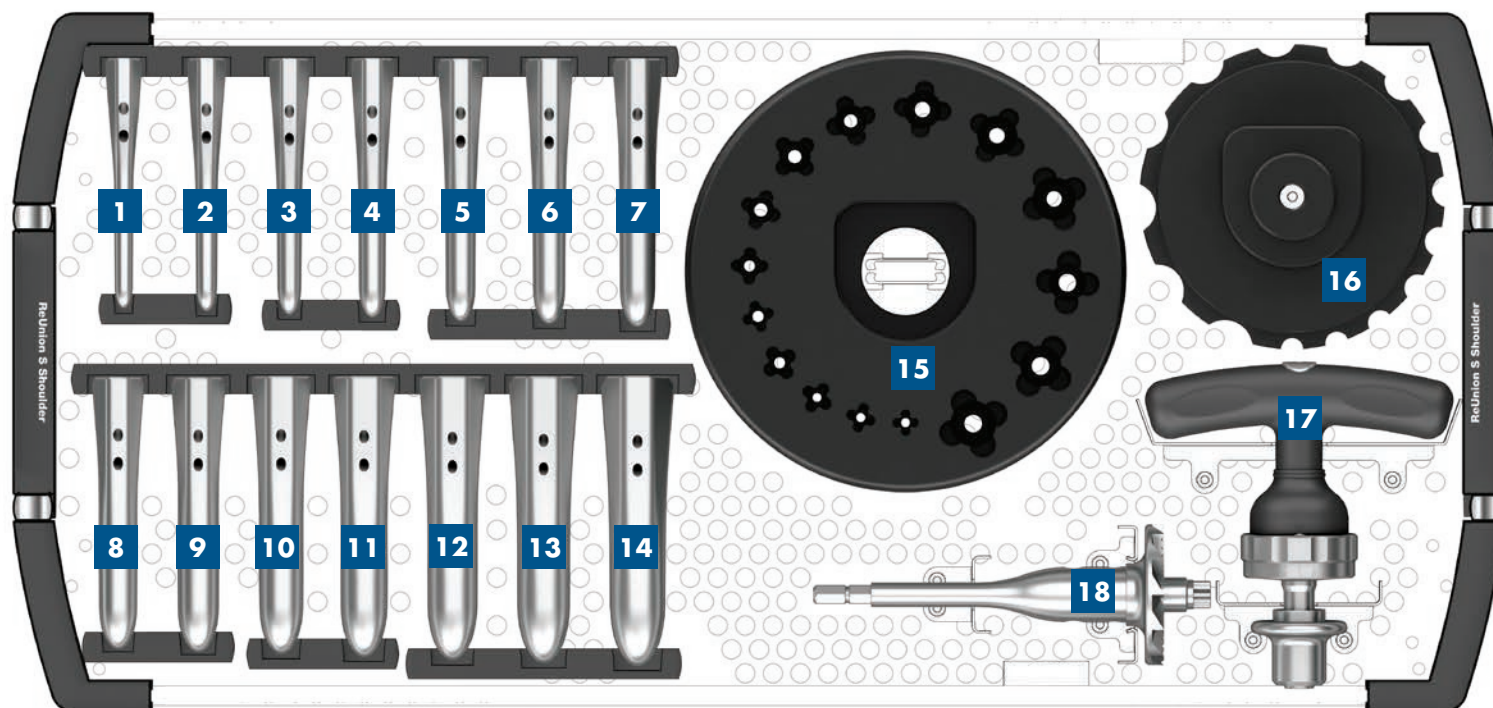

Ref #	Description	Size	Qty.
1 5901-3007	ReUnion S Humeral Broach	7mm	1
2 5901-3008	ReUnion S Humeral Broach	8mm	1
3 5901-3009	ReUnion S Humeral Broach	9mm	1
4 5901-3010	ReUnion S Humeral Broach	10mm	1
5 5901-3011	ReUnion S Humeral Broach	11mm	1
6 5901-3012	ReUnion S Humeral Broach	12mm	1
7 5901-3013	ReUnion S Humeral Broach	13mm	1
8 5901-3014	ReUnion S Humeral Broach	14mm	1
9 5901-3015	ReUnion S Humeral Broach	15mm	1
10 5901-3016	ReUnion S Humeral Broach	16mm	1

Ref #	Description	Size	Qty.
11 5901-3017	ReUnion S Humeral Broach	17mm	1
12 5901-3018	ReUnion S Humeral Broach	18mm	1
13 5901-3019	ReUnion S Humeral Broach	19mm	1
14 5901-3020	ReUnion S Humeral Broach	20mm	1
15 5901-4005	ReUnion S Humeral assembly block - lower deck		1
16 5901-4006	ReUnion S Humeral assembly block - upper deck		1
17 5901-1121	Modular ratcheting T-handle		1
18 5901-1181	Humeral calcar planar	Medium	1
	5901-1223	ReUnion S Shoulder Case	1



System components – ReUnion S Shoulder System

ReUnion S Press-fit Humeral Stem(s)

Ref #	Description	Diameter (distal)	Length
5567-P-3007	ReUnion S Press-fit Humeral Stem	7mm	91mm
5567-P-3008	ReUnion S Press-fit Humeral Stem	8mm	92mm
5567-P-3009	ReUnion S Press-fit Humeral Stem	9mm	93mm
5567-P-3010	ReUnion S Press-fit Humeral Stem	10mm	94mm
5567-P-3011	ReUnion S Press-fit Humeral Stem	11mm	95mm
5567-P-3012	ReUnion S Press-fit Humeral Stem	12mm	96mm
5567-P-3013	ReUnion S Press-fit Humeral Stem	13mm	97mm
5567-P-3014	ReUnion S Press-fit Humeral Stem	14mm	98mm
5567-P-3015	ReUnion S Press-fit Humeral Stem	15mm	99mm
5567-P-3016	ReUnion S Press-fit Humeral Stem	16mm	101mm
5567-P-3017	ReUnion S Press-fit Humeral Stem	17mm	102mm
5567-P-3018	ReUnion S Press-fit Humeral Stem	18mm	103mm
5567-P-3019	ReUnion S Press-fit Humeral Stem	19mm	104mm
5567-P-3020	ReUnion S Press-fit Humeral Stem	20mm	105mm

ReUnion S Cemented Humeral Stem(s)

Ref #	Description	Diameter (distal)	Length
5567-C-3006	ReUnion S Cemented Humeral Stem	6mm	89mm
5567-C-3007	ReUnion S Cemented Humeral Stem	7mm	91mm
5567-C-3008	ReUnion S Cemented Humeral Stem	8mm	92mm
5567-C-3009	ReUnion S Cemented Humeral Stem	9mm	93mm
5567-C-3010	ReUnion S Cemented Humeral Stem	10mm	94mm
5567-C-3011	ReUnion S Cemented Humeral Stem	11mm	95mm
5567-C-3012	ReUnion S Cemented Humeral Stem	12mm	96mm
5567-C-3013	ReUnion S Cemented Humeral Stem	13mm	97mm
5567-C-3014	ReUnion S Cemented Humeral Stem	14mm	98mm
5567-C-3015	ReUnion S Cemented Humeral Stem	15mm	99mm
5567-C-3016	ReUnion S Cemented Humeral Stem	16mm	101mm
5567-C-3017	ReUnion S Cemented Humeral Stem	17mm	102mm
5567-C-3018	ReUnion S Cemented Humeral Stem	18mm	103mm

A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate the breadth of Stryker product offerings.

A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: ReUnion, Stryker. All other trademarks are trademarks of their respective owners or holders.

Content ID: RU-TLC-3, 02-2019
Copyright © 2019 Stryker



Manufactured by:

Stryker GmbH
Bohnackerweg 1
2545 Selzach
Switzerland

stryker.com